



Conductivity Sensor 4319

is a compact fully integrated sensor for measuring the electrical conductivity of seawater. It is designed to be used with SeaGuard or SmartGuard datalogger using AiCaP CANbus or as stand-alone sensor using RS-232

Advantages:

- Smart Sensor for easy integration with SeaGuard and SmartGuard
- Direct readout of engineering data
- Internal pressure never exceeds 1 bar therefore electronics and sensors are unaffected by sea depth
- Rugged and robust with low maintenance needs
- Output format AiCaP CANbus, RS-232
- 3 depth ranges available max. 6000 meters

Conductivity is a key parameter for in-situ determination of several fundamental physical properties of seawater.

For seawater, the ability to conduct electrical current is mostly dependent on temperature and the amount of inorganic dissolved solids. This means that, together with temperature and depth information, a good estimate of the salinity may be determined.

Salinity is defined as the concentration of dissolved solids. Other important properties of seawater are again dependent on the salinity. Among these are the density and the speed of sound.


The Conductivity Sensor 4319 is based on an inductive principle. This provides for stable measurement without electrodes that are easily fouled and may wear out in the field.

Utilization of miniature components have made it possible to integrate all the required electronics.

The Conductivity Sensor outputs data in AiCaP CANbus and RS-232. Output parameters are conductivity and temperature in AiCaP and conductivity, temperature, salinity, density and sound speed in RS-232. Data can be presented in engineering units or raw data.

The SmartGuard datalogger and the Smart sensors are interfaced by means of a reliable CANbus interface (AiCaP), using XML for plug and play capabilities.

The Smart sensors can be mounted directly on the top end plate of the Aanderaa SmartGuard, in a String System node or connected to the SmartGuard and are automatically detected and recognized.

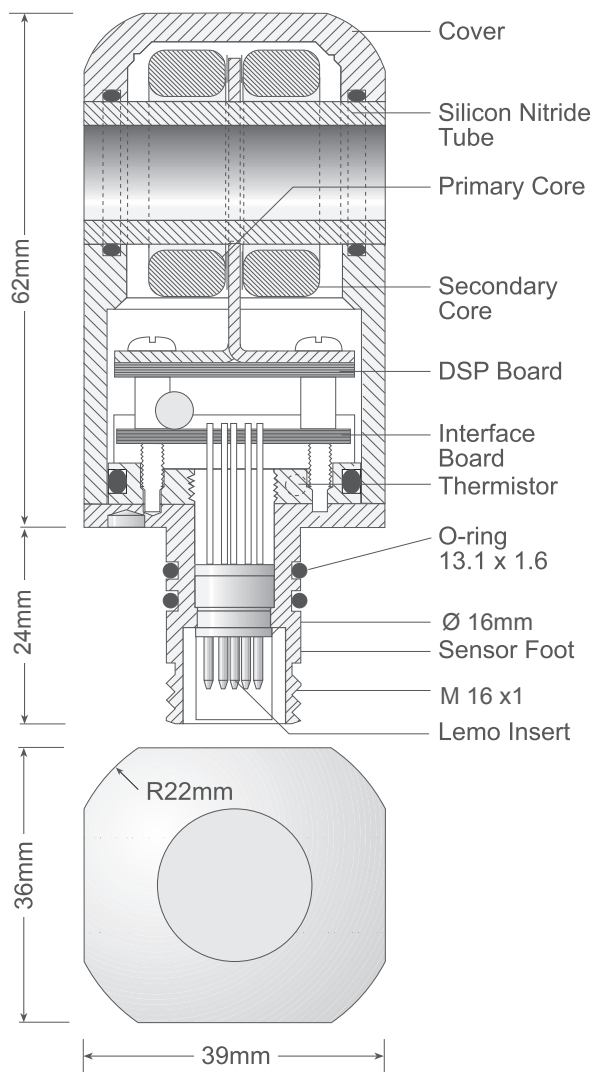

PIN CONFIGURATION

Receptacle, exterior view; pin = • bushing = ◦

CAN_H	4	5	NCE
NCG	3	6	BOOT_EN
NCR	9	10	CAN_L
Gnd	2	7	RS-232 RXD
Positive supply	1	8	RS-232 TXD

The 10-pin receptacle in the sensor foot mates with Aanderaa SP (Sensor Plug) giving access to both outputs. In RS-232 mode, use Sensor Cable 4865 for connection to a Personal Computer (PC). Cable 4865 is furnished with a watertight 10-pin SP-plug at the sensor end. An additional USB plug is used for providing power to the sensor.

Conductivity:

Range:	0–7.5S/m (0–75mS/cm)
Resolution:	0.0002S/m (0.002mS/cm)
Accuracy:	
4319A	±0.005S/m (±0.05mS/cm)
4319B	±0.0018S/m (±0.018mS/cm)
Response Time (90%):	<3s ⁽¹⁾

Temperature:

Range:	-5–40°C (23–104°F) ⁽²⁾
Resolution:	0.01°C (0.018°F)
Accuracy:	±0.05°C (0.09°F)/ (±0.1°C (0.18°F) for interval <30s.)
Response Time (63%):	<10 seconds

Output format:

AiCaP CANbus, RS-232

Output Parameter:

AiCaP:	Conductivity, temperature
RS-232:	Conductivity, temperature, salinity, density and sound of speed
Sampling interval:	2 sec – 255 min

Supply voltage:

5 to 14VDC

Current drain:

Average:	0.16 +48mA/S where S is sampling interval in seconds
Maximum:	100mA
Quiescent:	0.16mA

Operating depth:

Shallow Water (SW):	0–300m (0–984.3ft)
Intermediate Water (IW):	0–3000m (0–9843ft)
Deep Water (DW):	0–6000m (0–19690ft)

Electrical connection:

10-pin receptacle mating
SP-plug

Dimension (WxDxH):

36 x 39 x 86mm
(1.4"x1.5"x3.4")

Weight:

240g (8.466oz)

Materials:

Epoxy coated titanium

Accessories, not included:

Resistor Set 3719 for
functional test
Sensor Cable 4762,4865
Patch Cable 4999,3880L
Set-up and Config. Ca-
ble 3855⁽³⁾

⁽¹⁾ Dependant on flow through cell bore

⁽²⁾ Calibrated range is 0 to 36°C (32–96.8 °F)

⁽³⁾ Laboratory use only

The above specifications are for the stand-alone sensor only, not the installation it is utilized with.

Specifications subject to change without prior notice.



Visit our Web site for the latest version
of this document and more information

www.aanderaa.com

Aanderaa is a trademark of Xylem Inc. or one of its subsidiaries.
© 2016 Xylem, Inc. D369 August 2016

Aanderaa Data Instruments AS
Sanddalsringen 5b, P.O. Box 103 Midtun,
5843 Bergen, Norway
Tel +47 55 60 48 00
Fax +47 55 60 48 01